


Traceability scheme – CSM mass lab

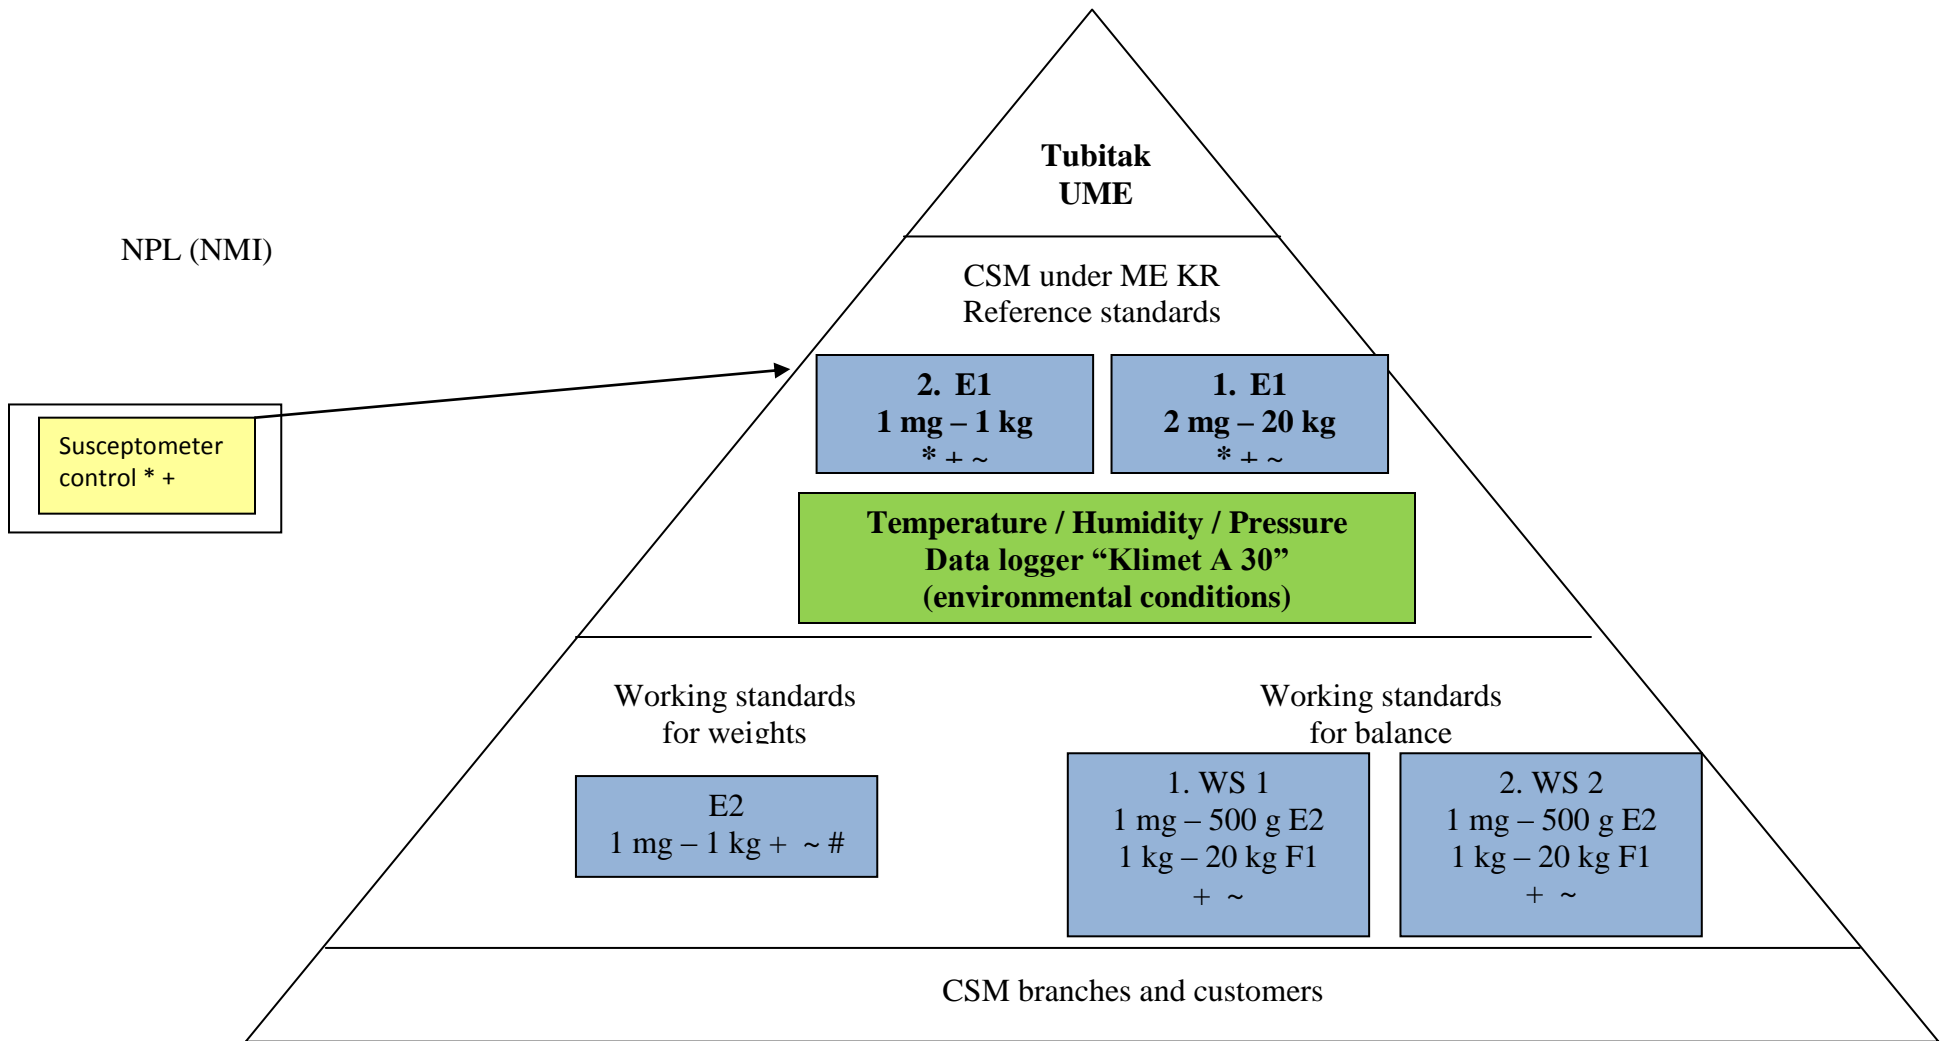

* calibration at NMI, listed at BIPM data base for the required measuring range (when application for CMC entries intended)
+ calibration at calibration laboratory, accredited according to ISO/IEC 17025 for the required measuring range (DAkkS,NVLAP)
internal calibration (when accredited)
~ intermediate check