


Laboratory of national standards of CSM under ME KR		Edition #	3
P 6.5_ A1/03	Traceability matrix	Date of issue	30.04.2019
		Page	1 from 2

Traceability scheme – CSM lenght lab

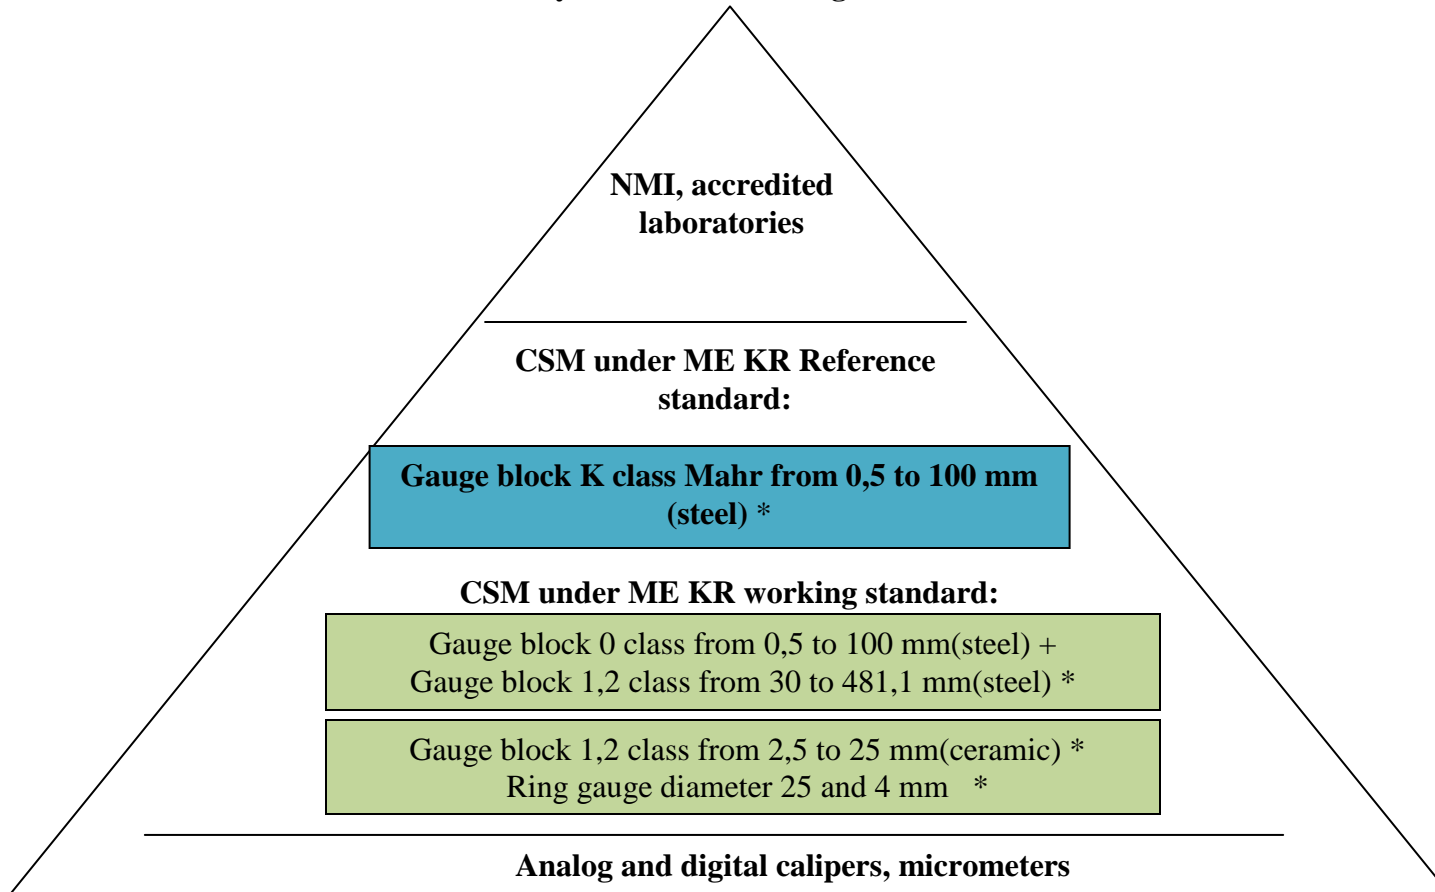


* calibration at NMI, listed at BIPM data base for the required measuring range (when application for CMC entries intended)
+ calibration at calibration laboratory, accredited according to ISO/IEC 17025 for the required measuring range (DAkkS, KCA)
internal calibration (when accredited)
~ intermediate check

Date	30.05.2019	Version	2	Update made by	Esenamanova Zh.
-------------	------------	----------------	---	-----------------------	-----------------

Laboratory of national standards of CSM under ME KR		Edition #	3
P 6.5_ A1/03	Traceability matrix	Date of issue	30.04.2019
		Page	2 from 2

Traceability scheme – CSM lenght lab

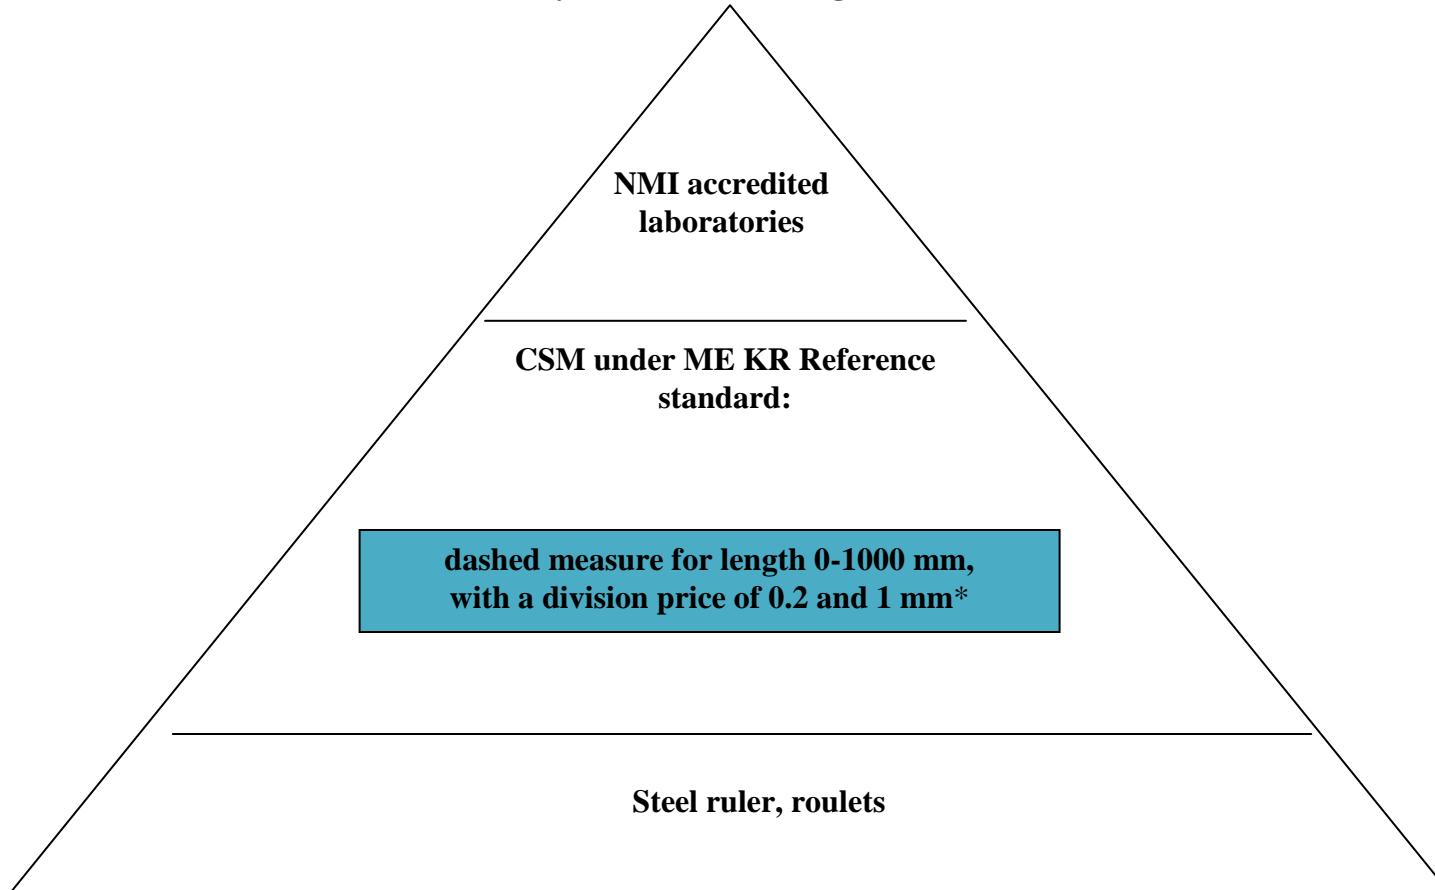

- * calibration at NMI, listed at BIPM data base for the required measuring range (when application for CMC entries intended)
- + calibration at calibration laboratory, accredited according to ISO/IEC 17025 for the required measuring range (DAkkS, KCA)
- # internal calibration (when accredited)
- ~ intermediate check

Date	30.05.2019	Version	2	Update made by	Esenamanova Zh.
-------------	------------	----------------	---	-----------------------	-----------------